


pardo NewCare V3 Bed

QUICK REFERENCE SHEET

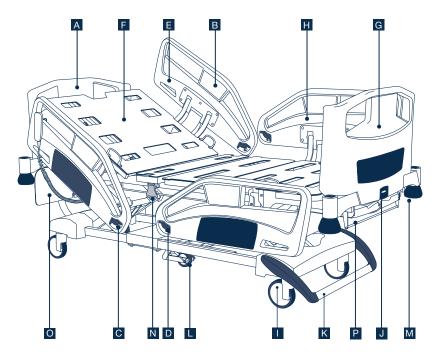

BED'S COMPONENTS

А	Removable headboard	-1	Wheels Ø15 cm.
В	Side rails membrane control	J	Headboard and footboard unlocking
С	Backrest tilting indicator	К	Braking pedal
D	Trend / Reverse Trend tilting indicator	L	5 th wheel
E	Backrest side rails	М	Protection discs
F	HPL mattress platform	N	Emergency CPR
G	Removable footboard	0	Anchored headboard
Н	Legrest side rails	Р	Extension bed base

www.pardo.es TECHNICAL SERVICE CENTRE (+34) 976 300 033

OTHER FUNCTIONS

Side Rails (1):


- Raising the rail: Pull the rail upwards until it is immobilised in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.


Emergency CPR (2):

Activate either of the two levers located in the middle of bed base, accompanying it in turn as it lowers.

Braking pedal (3):


- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in intermediate position.
- Activating 5th or steering wheel: Pedal in raised position.







Raising the rails

Lowering the rails









Emergency CPR

Free movement Brake

Steering or 5th wheel

CLEANING

Daily cleaning and disinfection with at least 1000ppm concentration of chlorine solutions:

- Rails. Head board. Foot board. Cleaning and disinfection after a patient leaves or before a transfer:
- Mattress platform area. Chassis of the bed. Thorough cleaning and disinfection every two
- Support and lifting area of the bed.


Maintenance

Always check the correct state of:


- Electrical wiring
- Wheels.
- Braking mechanisms.




For more information, please consult the use and maintenance manual.




Patient membrane with locking




Patient hand control with light




Nursing hand control



Membrane side rails



Patient control for motorised foot section



Nursing membrane with locking

INSTRUCTIONS OF USE

Α	Rise backrest	Ν	Cardiac chair position
В	Lower backrest	0	Light under bed
С	Rise mattress platform	Р	Emergency CPR
D	Lower mattress platform	Q	On/Off Button (to active membranes)
Е	Rise legrest	R	Safe bed exit position
F	Lower legrest	S	30° tilting backrest position
G	Rise all sections simultaneously (autocontour)	Т	30° tilting backrest Led indicator
Н	Lower all sections simultaneously (autocontour)	U	Low position Led indicator
I	Reverse Trend	V	Rise foot section
J	Trend	W	Battery indicator
K	Locking movements	Χ	Explorer position (maximum height)
L	Indicator Led of locked movements	Υ	Emergency trend position
М	Flat Position (lower all sections simultaneously)	Z	Lower foot section

















SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

