




# NewCare V2 Timotion Bed

## QUICK REFERENCE SHEET

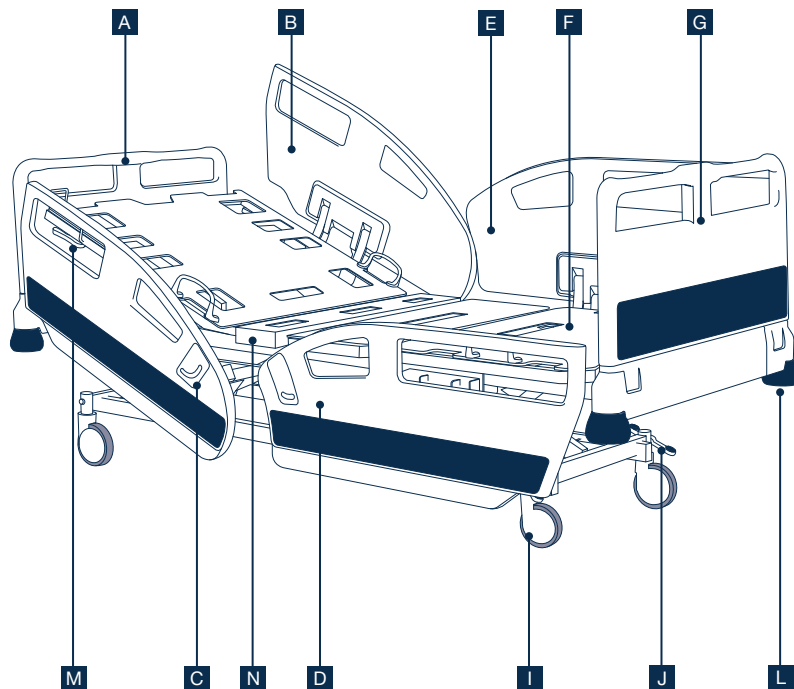

### BED'S COMPONENTS

A	Removable curved headboard	G	Removable curved footboard
B	Backrest side rails	I	Integral wheels Ø15 cm.
C	Backrest tilting indicator	J	Braking pedal
D	Trend / Reverse Trend tilting indicator	L	Protection discs
E	Legrest side rails	M	Emergency CPR
F	HPL mattress platform	N	Sheet steel central section

### OTHER FUNCTIONS

#### Side Rails (1):


- Raising the rail: Pull the rail upwards until it is immobilised in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.

#### Centralised braking system (3):


- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in intermediate position.
- Activating steering wheel: Pedal in raised position.

#### Emergency CPR (2):



- Activate either of the two levers located under the headrest module, accompanying it in turn as it lowers.




Raising side rails

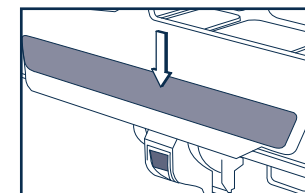


Lowering side rails

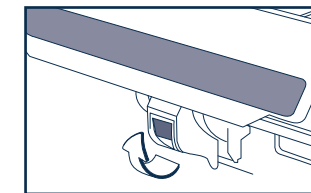


Emergency CPR



Brake



Free movement



Steering wheel

### CLEANING

Daily cleaning and disinfection with at least 1000ppm concentration of chlorine solutions:

- Rails. Head board. Foot board.

Cleaning and disinfection after a patient leaves or before a transfer:

- Mattress platform area. Chassis of the bed.

Thorough cleaning and disinfection every two months:

- Support and lifting area of the bed.

### MAINTENANCE

Always check the correct state of:

- Electrical wiring
- Wheels.
- Braking mechanisms.



# CONTROLS

## INSTRUCTIONS OF USE


A	Rise backrest	I	Reverse Trend
B	Lower backrest	J	Trend
C	Rise mattress platform	K	Locking movements
D	Lower mattress platform	L	Locking movements led indicator
E	Rise legrest	N	Cardiac chair position
F	Lower legrest	P	Emergency CPR
G	Rise backrest and legrest simultaneously ( <i>autocontour</i> )	W	Battery indicator
H	Lower backrest and legrest simultaneously ( <i>autocontour</i> )	Y	Emergency trend position

## LOCK AND UNLOCK OF PATIENT CONTROL


Function locking is used to disable bed basic functions, mainly to lock movements which has to be done under medical guidance.

To Lock and Unlock the bed functions, only extract or insert the locking key. This key is localised at the bottom of the wired control.


- **Unlock:** Insert the locking key on the lateral of wired control. The Indicators (L) are lighted on green colour.
- **Lock:** Extract the locking key on the lateral of wired control. The Indicators (L) are lighted on red colour.

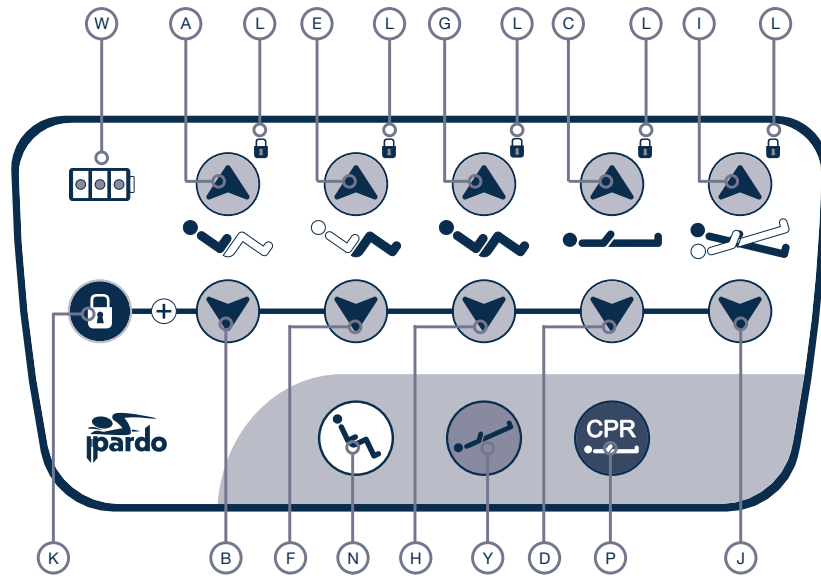

Wired nursing control

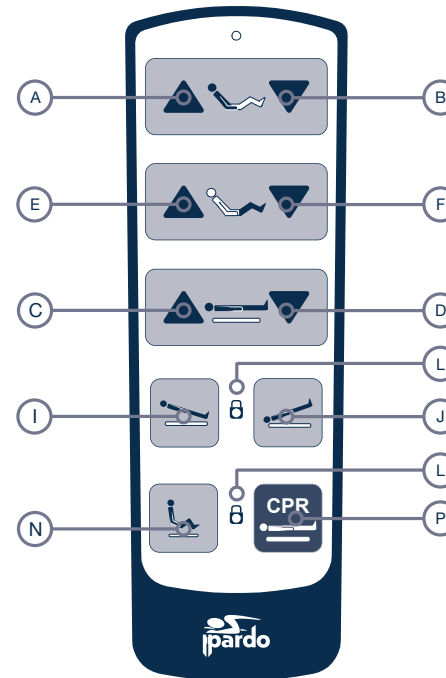

Patient control with locking

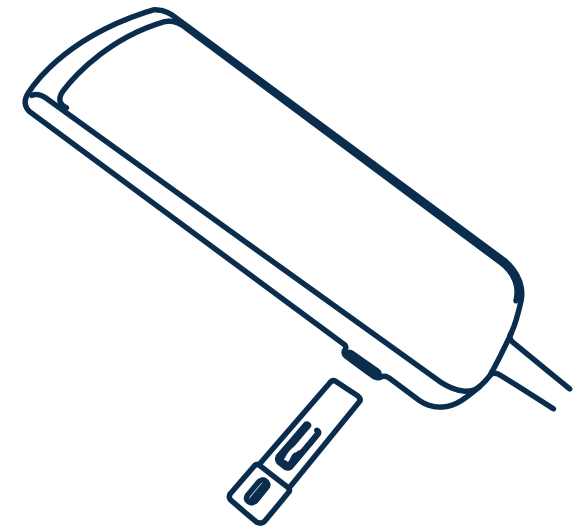

Locking key of patient control



### SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

