New Cartago armchair

Quick reference sheet

Armchair components

A	Transfer handle	E	Double wheels Ø10 cm
B	Backrest	F	Legrest actuation lever
C	Armrest	G	Footrest
D	Seat	H	Legrest

Other functions of the armchair

Armrest

- Fold down: Raise the armrest and turn it backwards.
- Raise: Move the armrest forward until it returns to its original position.

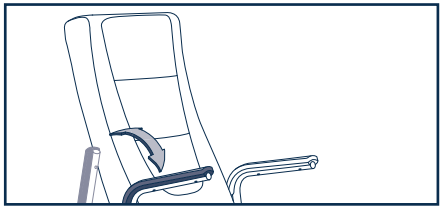

Armrest lifting

Wheels and braking system

- Brake: Press the pedal to its lowest position.
- Free movement: Lift the pedal with your foot until it is in its highest position.



Brake



Free movement

Cleaning

It is recommended to clean the unit with detergent and warm water. Do not use excessive amounts of liquid or abrasive cleaning products.

Daily cleaning and disinfection

- Backrest, seat, legrest, armrest and handle.

Cleaning and disinfection after a patient leaves or before a transfer:

- Backrest, seat, legrest, armrest, handle, footrest, operating levers.

Thorough cleaning and disinfection every two months:

- The whole chair.

Maintenance

Always check the correct condition of:

- Wheels.
- Braking mechanisms.
- Mechanical components for driving the backrest and legrest.

For more information, please consult the use and maintenance manual.

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | CódPCO700684_QuickSheet_NewCartago_EN_2020_rev01

Mechanical operation

Backrest adjustment

- Fold down the backrest: Move the lever located on the left side of the seat backwards and press on the backrest to the desired position.
- Raise backrest: Press the lever on the left side of the seat backwards and let it rise freely, without leaning on it or using any force.

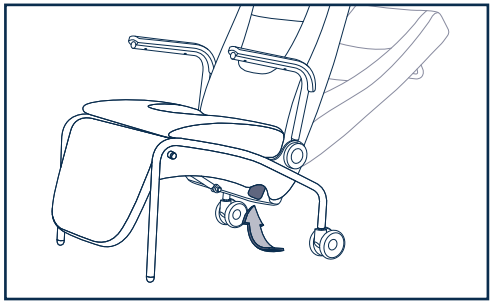

Backrest adjustment lever

Fold down backrest

Raise backrest

Legrest adjustment

- Extend: Move the lever located on the right side of the seat backwards and let the legrest rise freely until it is in the desired position.
- Fold down: Press the lever located on the right side of the seat and press the legrest down until it lowers to its original position.

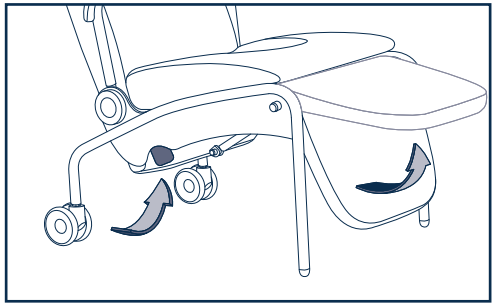

Extend legrest

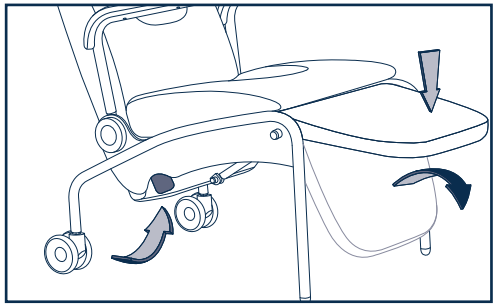

Fold down legrest

Accesories

Footrest

- When the version of the chair is with four wheels, there is the possibility of incorporating a footrest.
- To collect the footrest, turn the section of feet approximately 90º and rotate the entire assembly, using the leg of the chair as an axis.

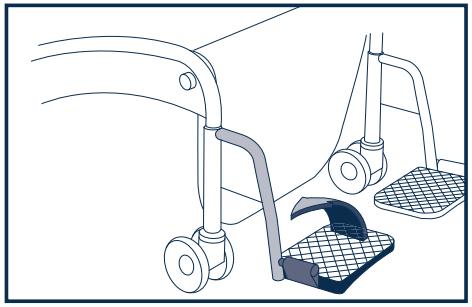

Extended footrest

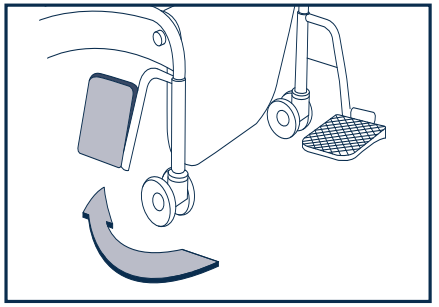

Fold down footrest

Armchair setup

Depending on the user for whom the chair is intended, patient or companion, it can be configured with different accessories:

- Patient version with transfer.
- Patient version with room mobility.
- Patient accompanying version.

Patient version with transfer.

Patient version with room mobility.

Patient accompanying version.

Industrias Hidráulicas Pardo S.L. has the following certificates

SAFETY WARNINGS

- Do not sit on the backrest to avoid lack of stability of the chair or breakage due to overweight. Handle the leg section carefully when lifting or folding it down in order to avoid crushing your hands.
- Do not sit on the armrest to avoid a lack of stability of the chair or breakage due to overweight.
- Handle the leg section carefully when lifting or picking it up in order to avoid crushing your hands.
- If the chair or the patient is not being transported, the brakes on all wheels must be activated as damage could occur if it were to move accidentally.

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)