Easo Bed

Quick reference sheet

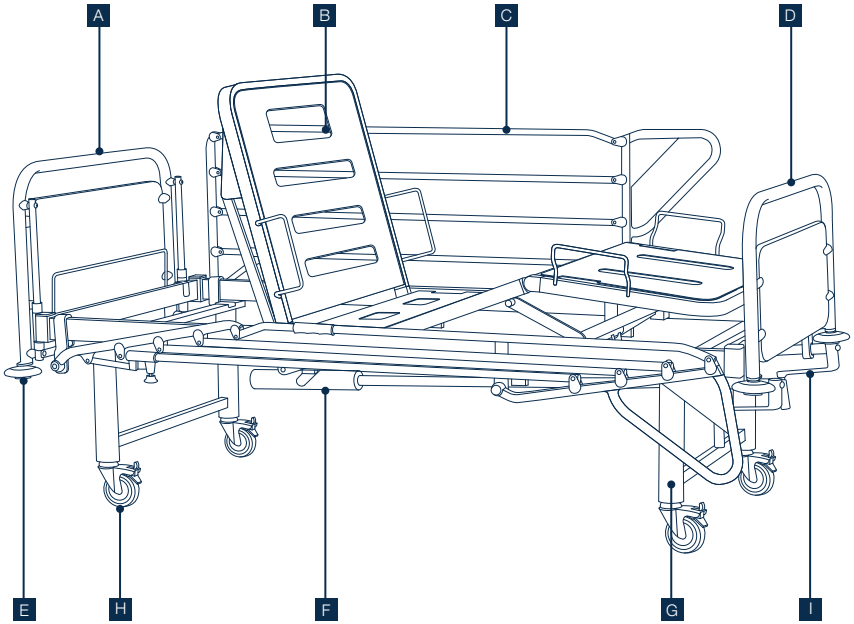

Bed's components

A	Headboard	F	Hydraulic bed lift
B	HPL mattress platform	G	Steel tube legs
C	Tube side rails	H	Sheet steel wheels
D	Footboard	I	Cranks
E	Protection discs		

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | Cód: PCO701557_QuickSheet_Easo_EN_2024

Other functions

4 Tube side rails:

- Rise side rails: Pull of the side rail towards headboard up (1) to hearing "click" from the lower handle (2), then the side rail is locked in highest position.
- Lower side rails: Unlock side rail lower handle pulling of it down (3). Fold the said rail (4) towards footboard taking it until lowest position where it remains locked.

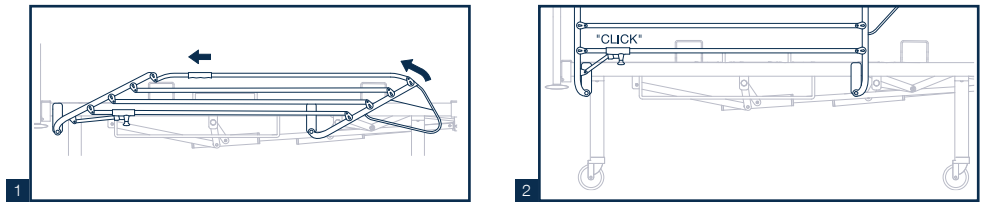

Rise side rails

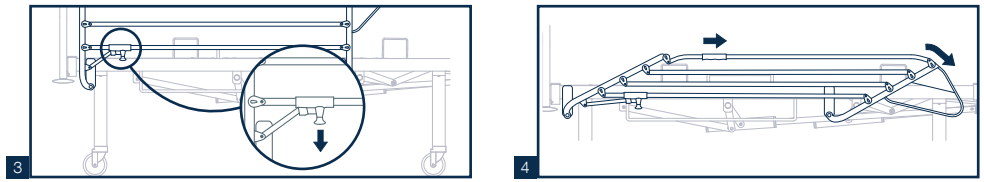

Lower side rails

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails, headboard, footboard.

Cleaning and disinfection after a patient leaves or before a transfer:

- Mattress platform area, chassis of the bed.

Thorough cleaning and disinfection every two months:

- The entire bed.

Maintenance

Always check the correct state of:

- Headboards and footboards.
- Legs, wheels and braking mechanisms.
- Mechanical body and bed drive components.

For more information, please consult the use and maintenance manual.

MOVEMENTS OF THE BED BODIES

Unlock crank:

- Pull the lever bed outwards (1).
- Direct it to its working position (2).
- Push the lever to the correct position.

Backrest section:

- Raise: Turn clockwise the left crank handle (3).
- Lower: Turn anticlockwise the left crank handle (4).

Legs section:

- Raise: Turn clockwise the right crank handle (5).
- Lower: Turn anticlockwise the right crank handle (6).

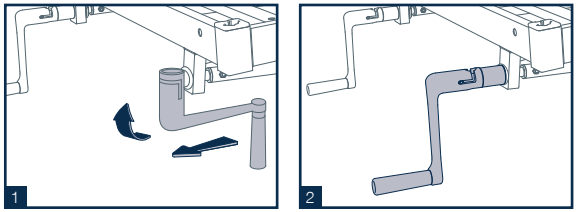

Unlock crank and working position

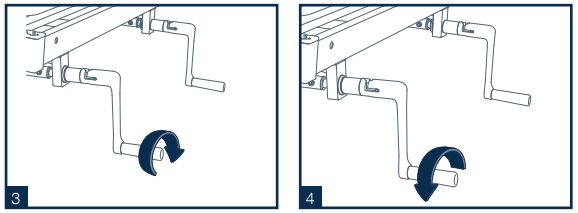

Raise backrest

Lower backrest

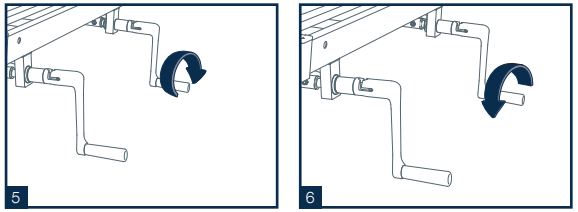

Raise extremities

Lower extremities

OTHER FUNCTIONS

Wheels with individual brake:

- The bed can be equipped with 4 metal castors (Ø12'5 cm or Ø10 cm) with individual brakes. Para activar el freno, pisar la palanca hasta su posición más baja. To activate the brake, push the lever to its lowest position. To deactivate it, lift the lever with your foot to its highest position.

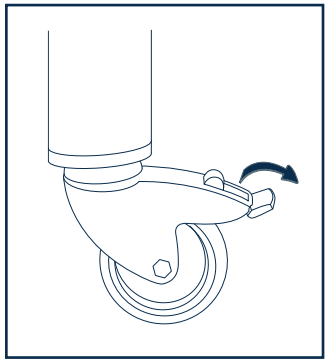

Wheels with individual brake

Industrias Hidráulicas Pardo S.L. company has the following certifications:

SAFETY WARNINGS

- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- There is a risk of tripping or falling if the handles are in the operating position. Remember to retract the handle after use..