NewCare Bed

Quick reference sheet

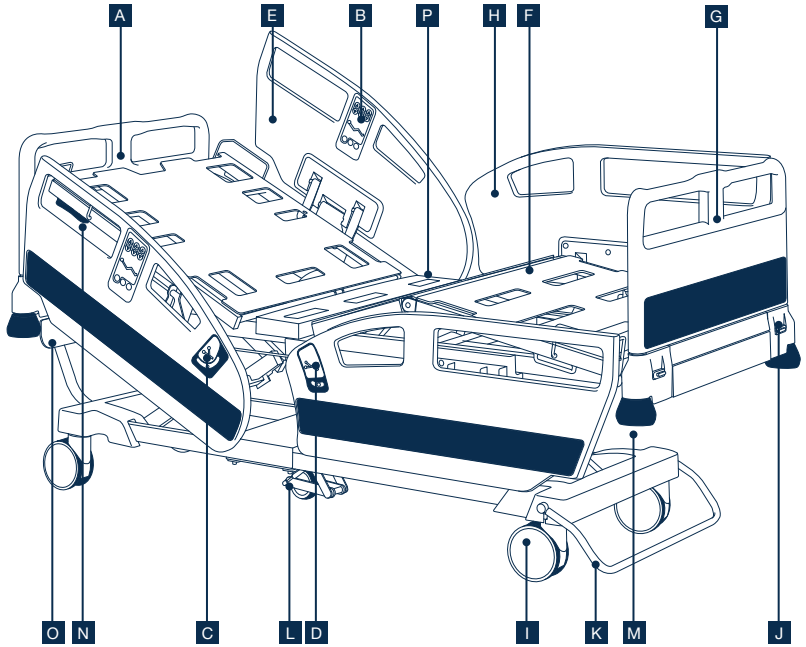

Bed's components

A	Removable curved headboard	I	Double wheels Ø15 cm
B	Side rails membrane control	J	Headboards and footboards unlocking
C	Backrest tilting indicator	K	Centralised braking system
D	Trend / Reverse Trend tilting indicator	L	Fifth wheel
E	Backrest side rails	M	Protection discs
F	HPL mattress platform	N	Emergency CPR
G	Removable curved footboard	O	Anchored headboard
H	Legrest side rail	P	Sheet steel central section

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | Cód:PCO729822_QuickSheet_NewCare_EN_2020_rev03

Other functions

Side rails (1):

- Raising the rail: Pull the rail upwards until it is locked in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.

Emergency CPR (2):

- Activate either of the two levers located under the headrest module, accompanying it in turn as it lowers.

Centralised braking system (3):

- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in the middle position.
- Activating the 5th or steering wheel: Pedal in raised position.

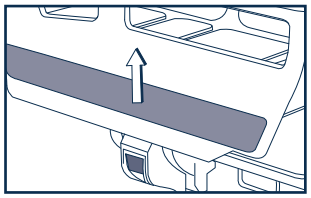

Rising the rails

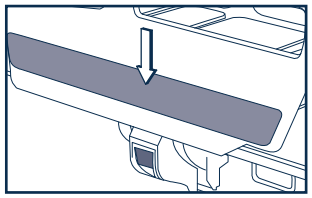

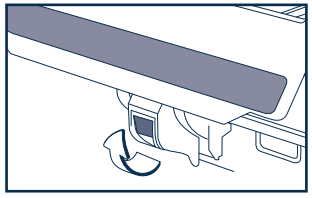

Lowering the rails

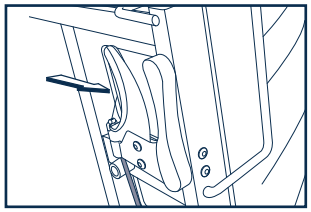

Emergency CPR



Brake



Free movement



Steering or 5th wheel

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails, headboard, footboard.

Cleaning and disinfection after a patient leaving or before a transfer:

- Mattress platform area, chassis of the bed.

Deep cleaning and disinfection every two months:

- Support and lifting area of the bed.

Maintenance

Always check the correct state of:

- Electrical wiring.
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

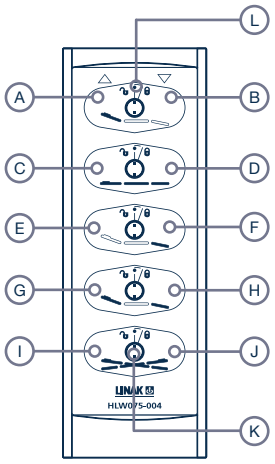

Patient hand control with locking

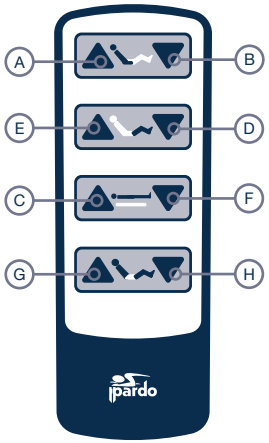

Patient hand control

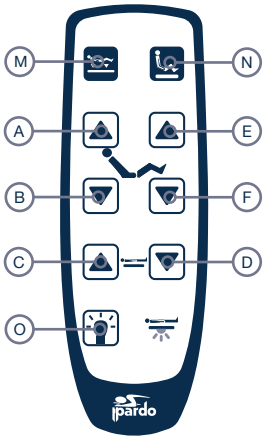

Patient hand control with light

INSTRUCTIONS OF USE

A	Rise backrest	J	Trendelenburg	T	30º backrest indicator led
B	Lower backrest	K	Locking movements	U	Low Position indicator led
C	Rise mattress platform	L	Indicator led of locked movements	V	Trendelenburg / Reverse Trendelenburg selector
D	Lower mattress platform	M	Flat position (lower all sections simultaneously)	W	Battery indicator
E	Rise legrest	N	Cardiac Chair position	X	Exploration Position (maximum height)
F	Lower legrest	O	Light under bed	Y	Emergency Trend position
G	Rise both simultaneously *(autocontour)*	P	Emergency CPR	Z	Nursing call
H	Lower both simultaneously *(autocontour)*	Q	Standby button		
I	Reverse Trendelenburg	R	Safety Exit position		

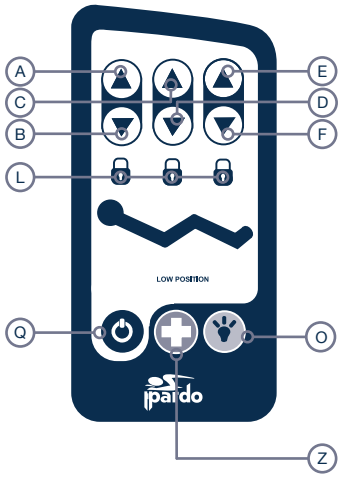

Membrane control

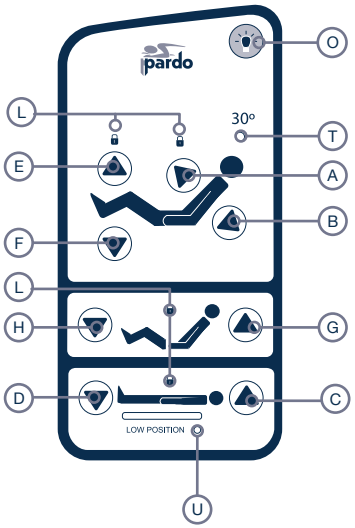

Patient mebranes

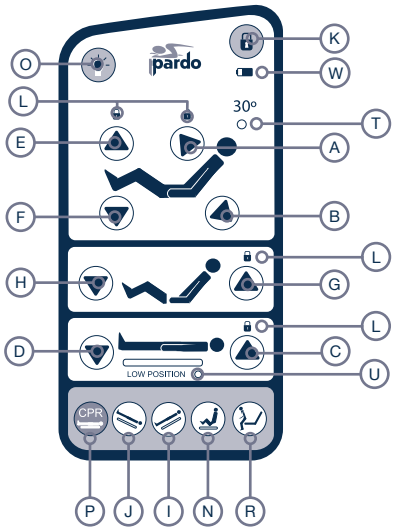

Nursing membranes

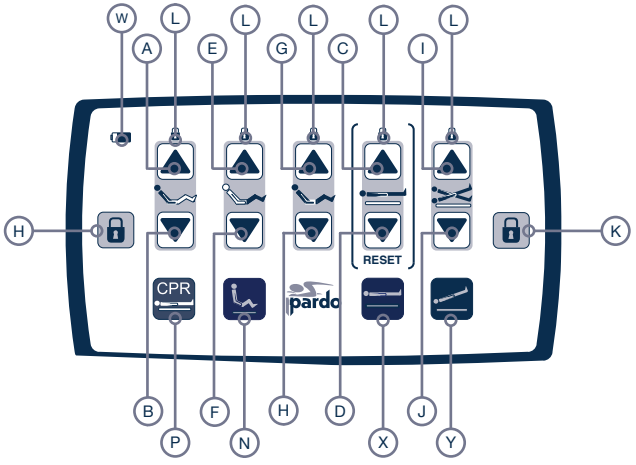

Nursing control

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD PRODUCTOS SANITARIOS · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.