# NewBabyCare Bed

## Quick reference sheet

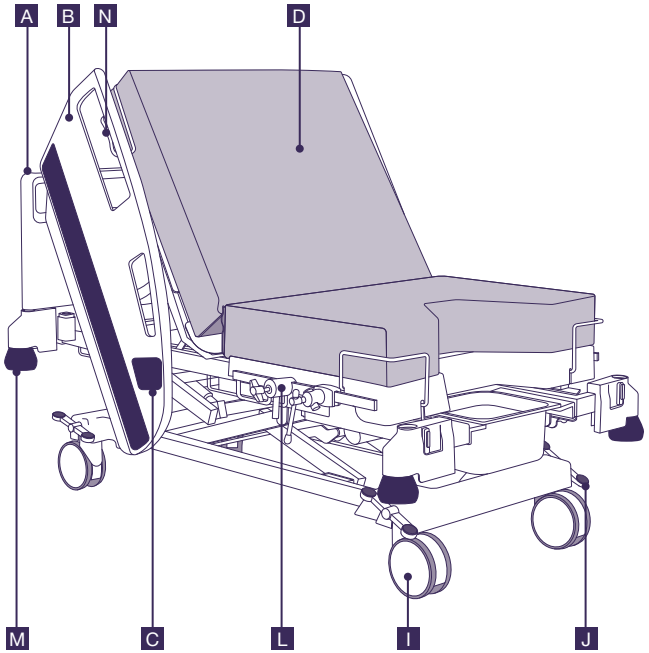


## Bed's components

| | | | |
|---|---|---|---|
| A | Removable curved headboard | J | Centralised braking pedal |
| B | Backrest side rails | L | Clamps for accessories |
| C | Backrest tilting indicator | M | Protection discs |
| D | Fixed mattress | N | Emergency CPR |
| I | Double wheels Ø15 cm | | |

## Typology of gynaecological accessories

**Non-epidural labor - High mechanical demand (1):**
- Upper extremities: Grip frame or handles.
- Lower extremities: "L" footrests.

**Epidural labor - Medium mechanical demand (2):**
- Upper extremities: Grip frame or handles.
- Lower extremities: Legrest.

**Observation - Low mechanical demand (3):**
- Upper extremities: Handles.
- Lower extremities: Footrests.

Grip frame

Grip frame


Handles


Handles


Handles


Footrests


"L" footrests

Legrest

## Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:
- Rails, headboard, footboard.

Cleaning and disinfection after a patient leaving or before a transfer:
- Mattress platform area, chassis of the bed.

Deep cleaning and disinfection every two months:
- Support and lifting area of the bed.

## Maintenance

Always check the correct state of:
- Electrical wiring.
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | CódPOO731371_QuickSheet_NewBabyCare_EN_2020_rev.03

## Other functions

Side rails (1):

- Raising the rail: Pull the rail upwards until it is locked in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.

Centralised braking pedal (2):

- Braking the bed: Pedal in low position.
- Free movement: Pedal in the horizontal position.
- Steering wheel: Pedal in raised position.

Emergency CPR (3):

- Activate either of the two levers located under the headrest module, accompanying it in turn as it lowers.

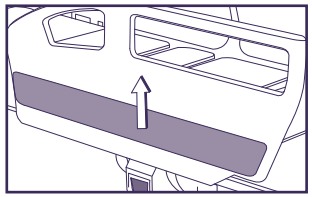

Rising the rails

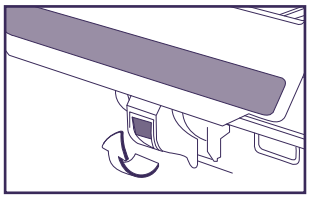

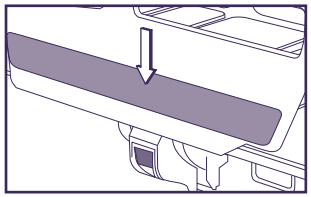

Lowering the rails

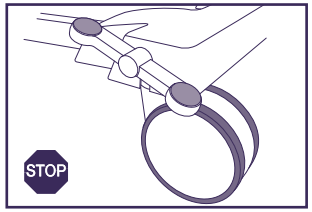


Brake

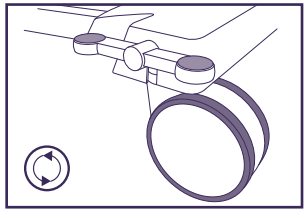

Free movement

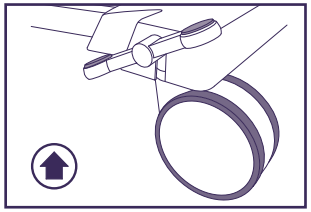

Steering



Emergency CPR

## Lock and unlock of patient control

Function locking is used to disable bed basic functions, mainly to lock movements which has to be done under medical guidance.

To Lock and Unlock the bed functions, only extract or insert the locking key. This key is localised at the bottom of the wired control.

- **Unlock:** Insert the locking key on the lateral of wired control. The Indicators (L) are lighted on green colour.
- **Lock**: Extract the locking key on the lateral of wired control. The Indicators (L) are lighted on red colour.

## Control

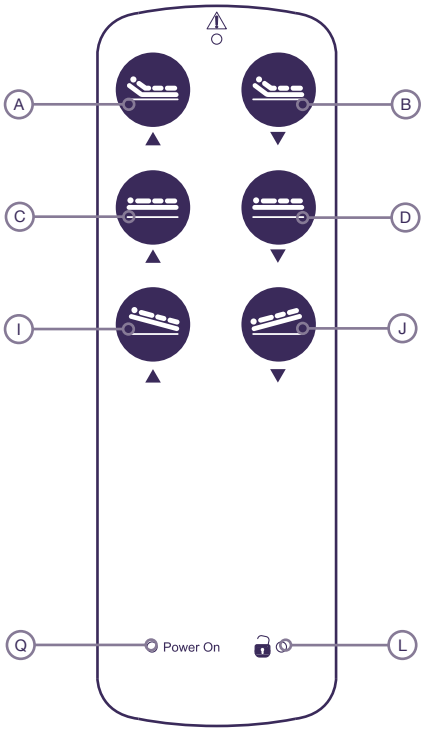


Patient control with locking

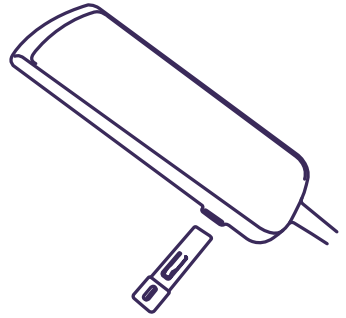

Locking key of patient control

## Instructions of use

| | |
|---|---|
| A | Rise backrest |
| B | Lower backrest |
| C | Rise mattress platform |
| D | Lower mattress platform |
| I | Reverse Trend |
| J | Trend |
| L | Indicator Led of locked movements |
| Q | Indicator Led of power function |

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD, GESTIÓN DEL SEGURIDAD Y SANITARIOS · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

### SAFETY WARNINGS

- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

pardo