Alzheimer 19/75 Bed

Quick reference sheet

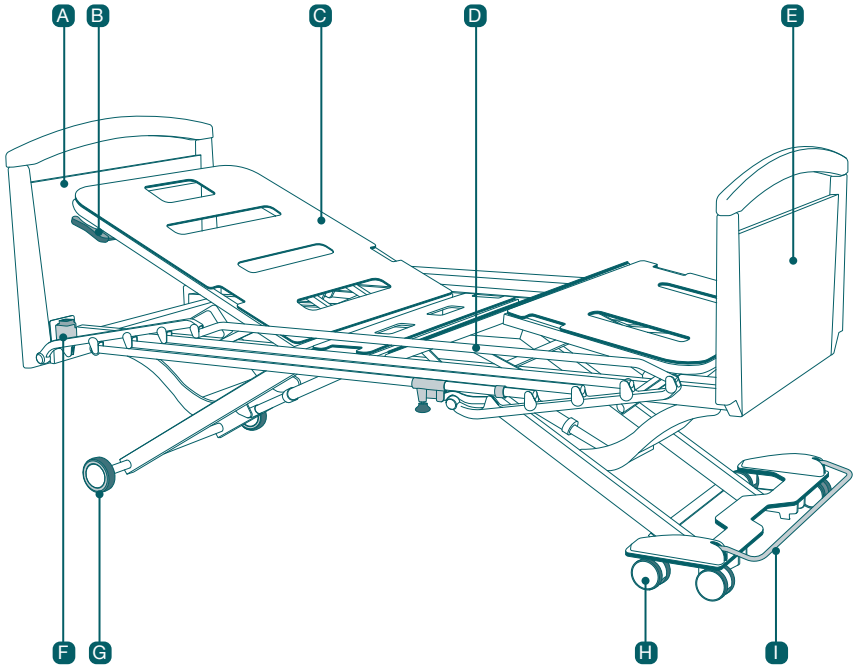

Bed's components

A	Screwed headboard	F	Soporte accesorios
B	Emergency CPR handle	G	Fixed wheels Ø10 cm
C	HPL mattress platform	H	Wheels Ø7,5 cm
D	4 tube side rails	I	Brake pedal
E	Screwed footboard		

Side rails

Four tube side rails:

- Rise side rails: Pull of the side rail towards headboard up to hearing "click" from the lower handle, then the side rail is locked in highest position.
- Lower side rails: Unlock side rail lower handle pulling of it down. Fold the said rail towards footboard taking it until lowest position where it remains locked.

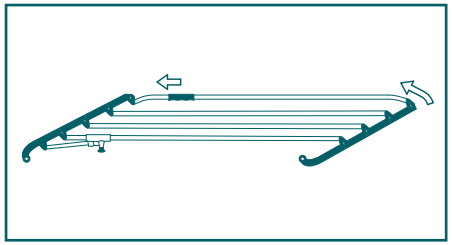

Rise side rails

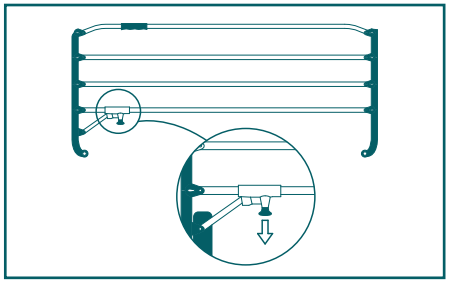

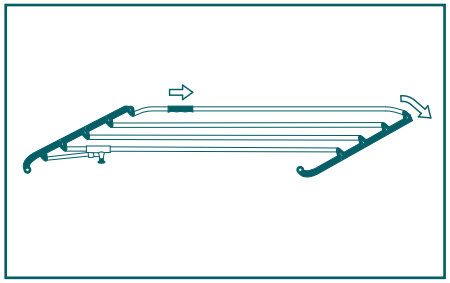

Lower side rails

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails, headboard, footboard.

Cleaning and disinfection after a patient leaving. or before a transfer:

- Mattress platform area, chassis of the bed, CPR handle, side rails, headboard, footboard.

Deep cleaning and disinfection every two months:

- Support and lifting area of the bed.

Maintenance

Always check the correct state of:

- Electrical wiring.
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | CódPOO735385_QuickSheet_Alzeimer-1975_EN_2024_rev01

Other functions

Multifunction pedal (1):

- Braking: Pedal in low position.
- Free moving: Pedal in horizontal position.

HPL mattress platform (2):

- Bed bases are easy to disassemble due to a piece that snaps into place by pressing it onto the bed frame until you hear a “click”.

Emergency CPR (3):

- Operate either of the two levers located on the underside of the backrest while accompanying it as it lowers.

Feet module positioning system (4):

- Raise inclination: Pull up the module.
- Descend incline: Raise the module slightly and lower it to the desired position.





Braking





Free movement

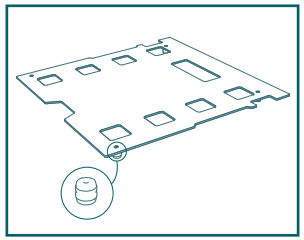

Mattress platform



CPR handles

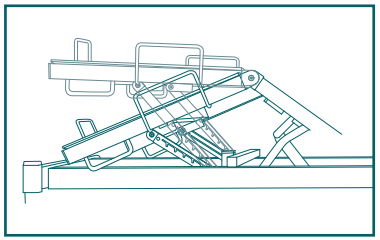

Feet module positioning

Lock and unlock of patient control

Function locking is used to disable bed basic functions, mainly to lock movements which has to be done under medical guidance.

To Lock and Unlock the bed functions, only extract or insert the locking key. This key is localised at the bottom of the wired control.

- **Unlock:** Insert the locking key on the lateral of wired control. The Indicators (L) are lighted on green colour.
- **Lock:** Extract the locking key on the lateral of wired control. The Indicators (L) are lighted on red colour.

Control

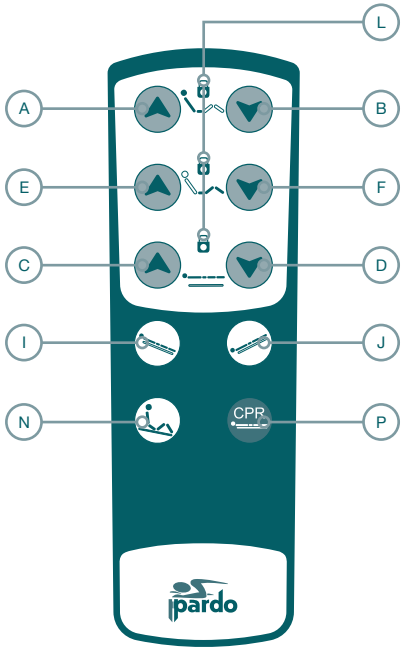

Wired patient control with locking

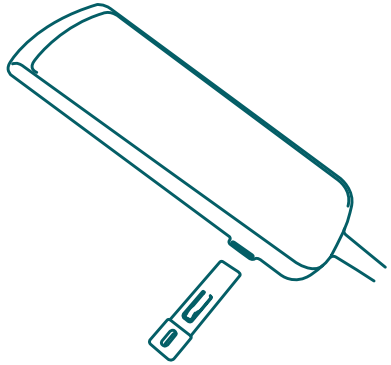

Movement locking key

Instructions of use

A	Rise backrest	I	Reverse Trendelenburg
B	Lower backrest	J	Trendelenburg
C	Rise mattress platform	L	Indicator Led of locked movements
D	Lower mattress platform	N	Cardiac Chair position
E	Rise legrest	P	Emergency CPR position
F	Lower legrest		

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD, GESTIÓN DEL SANEAMIENTO · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

SAFETY WARNINGS

- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

pardo

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)