Bora Med Bed

Quick reference sheet

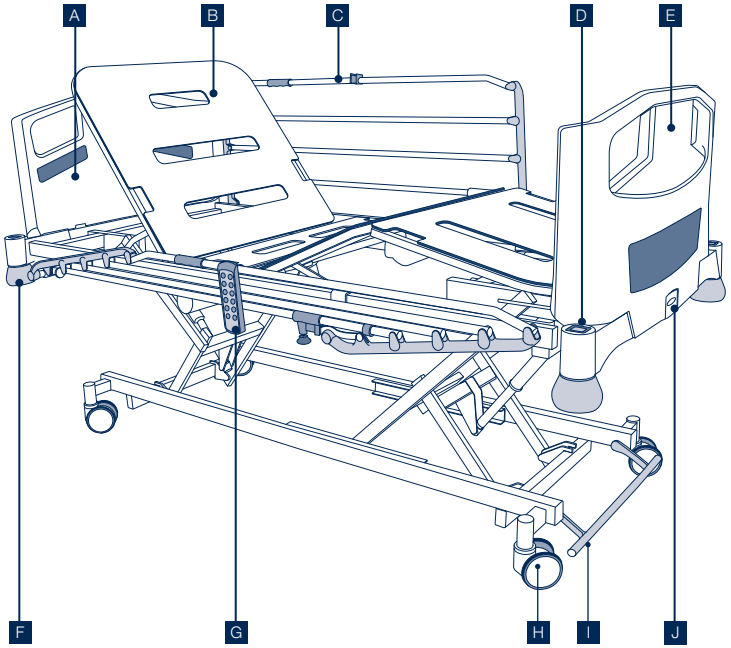

Bed's Components

A	Removable headboard	F	Protection discs
B	HPL mattress platform	G	Wired control
C	Tube side rails	H	Wheels Ø10 cm
D	Accessories support	I	Centralised braking system
E	Removable footboard	J	Headboard and footboard unlocking

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

mar 2026 | Cód:PCO748349_QuickSheet_BoraMed_EN_2020_rev04

Side Rails

Tube side rails:

- Rise side rails: Pull of the side rail towards headboard up to hearing "click" from the lower handle, then the side rail is locked in highest position.

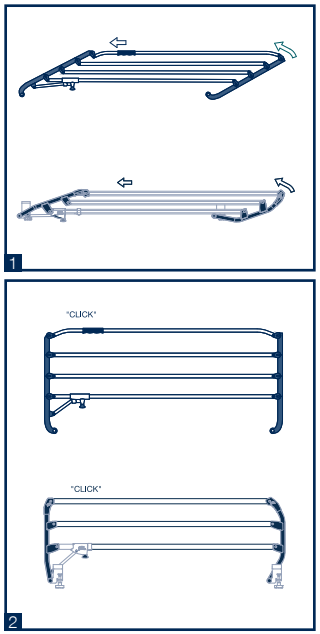

- Lower side rails: Unlock side rail lower handle pulling of it down. Fold the said rail towards footboard taking it until lowest position where it remains locked.

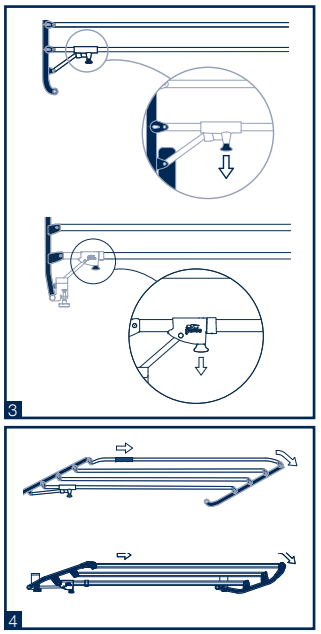

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails. Head board. Foot board.

Cleaning and disinfection after a patient leaves or before a transfer:

- Mattress platform area. Chassis of the bed.

Thorough cleaning and disinfection every two months:

- Support and lifting area of the bed.

Maintenance

Always check the correct state of:

- Electrical wiring.
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

Other functions

Braking pedal (1):

- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in intermediate position.
- Activating steering wheel: Pedal in raised position.

Emergency CPR (2):

- Activate either of the two levers located in the middle of bed base, accompanying it in turn as it lowers.

Extended bed base (3):

- Pull and turn the locking knobs 180º to unlocked the anchoring system.
- Pull the footboard until extended the bed base completely.
- Push the footboard until listening “click”.



Brake



Free movement



Steering wheel

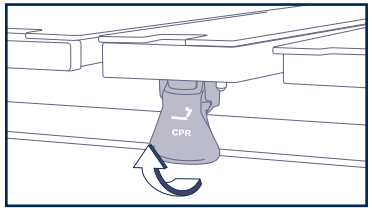

Emergency CPR







Extract the extended bed base

Controls

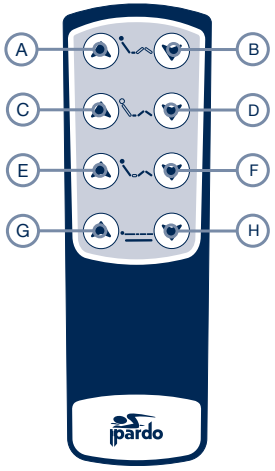

Patient control

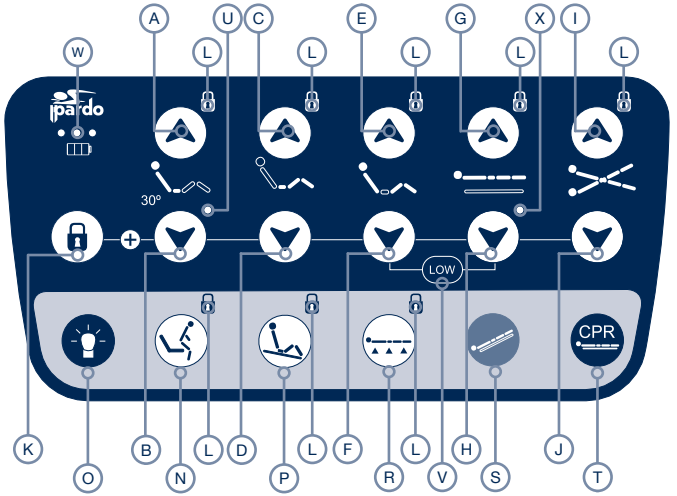

Nursing control

Instructions of use

A	Rise backrest	L	Indicator Led of locked movements
B	Lower backrest	N	Safe bed exit position
C	Rise legrest	O	Light under bed (2)
D	Lower legrest	P	Cardiac chair position
E	Rise all sections simultaneously *(autocontour)*	R	Exploration position (maximum height)
F	Lower all sections simultaneously *(autocontour)*	S	Emergency Trend position
G	Rise mattress platform	T	Emergency CPR
H	Lower mattress platform	U	Led indicator for backrest at 30º
I	Reverse Trend	V	Low Positon (1)
J	Trend	W	Led indicator for battery
K	Locking movements	X	Led indicator for low position

(1) Press simultaneity F+H, when the mattress platform is on minimum height.

(2) Only in case the bed incorporates it.

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD DISTRIBUCIÓN SANITARIOS · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)