Elita Med Bed

Quick reference sheet

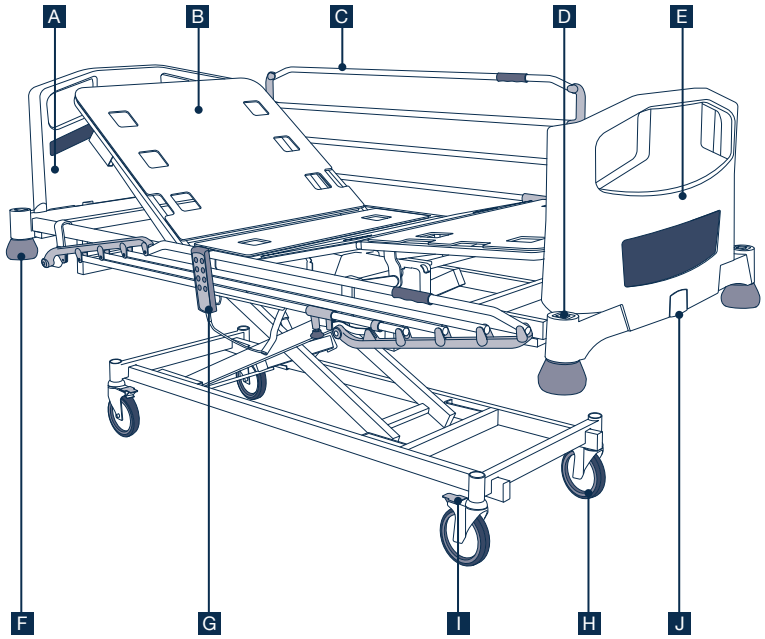

Bed's components

A	Removable headboard	F	Protection discs
B	HPL mattress platform	G	Patient control
C	4 tube side rails	H	Wheels Ø15 cm.
D	Accessories supports	I	Individual braking pedal
E	Removable footboard	J	Headboard and footboard unlocking

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | Cód:PCO752809_QuickSheet_ElitaMed_EN_2020_rev02

Side rails

Four tube side rails:

- Rise side rails: Pull of the side rail towards headboard up to hearing "click" from the lower handle, then the side rail is locked in highest position.
- Lower side rails: Unlock side rail lower handle pulling of it down. Fold the said rail towards footboard taking it until lowest position where it remains locked.

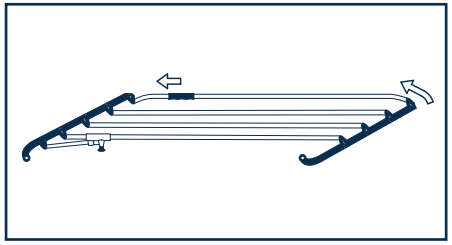

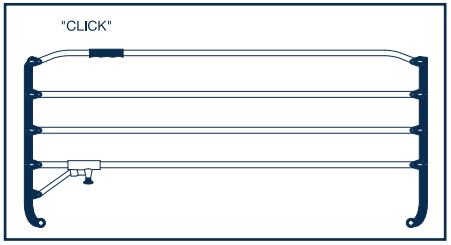

Rise side rails

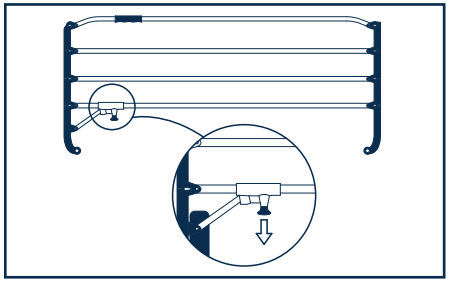

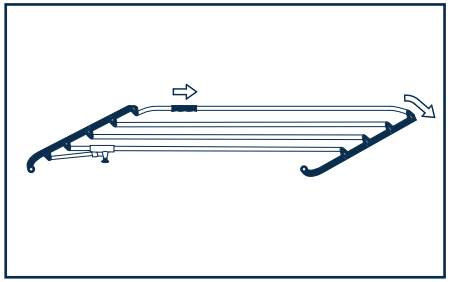

Lower side rails

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails. Head board. Foot board.

Cleaning and disinfection after a patient leaves or before a transfer:

- Mattress platform area. Chassis of the bed.

Thorough cleaning and disinfection every two months:

- Support and lifting area of the bed.

Maintenance

Always check the correct state of:

- Electrical wiring
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

Other functions

Braking pedal (1):

- Braking the bed: Pedal in the lowest position.
- Moving the bed: Pedal in the highest position.

Emergency CPR (2):

- Activate the lever located in the centre section of double compact actuator, accompanying the backrest module while descending.

Head/footboard with locking system (3):

- Placement: Insert the footboard anchors into the corner holes, pressing downwards, until they fit.
- Removal: Activate the lever located in the center of the headboard/footboard to unlock it. Holding the footboard, rise it vertically until it is removed.



Brake



Free movement

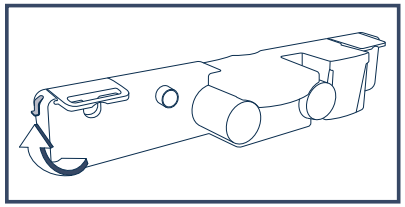

Emergency CPR

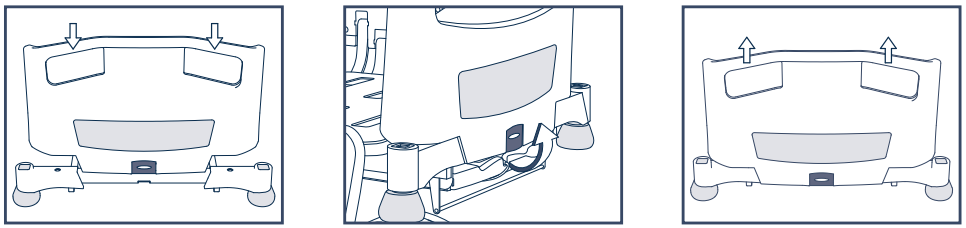

Placement / Removal of headboard and footboard

Controls

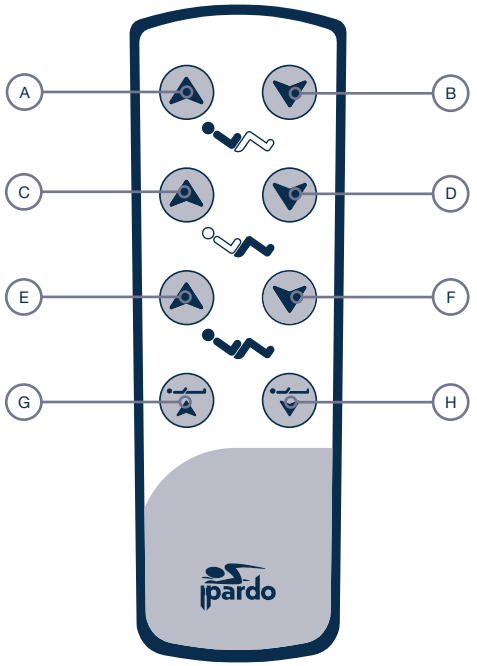

Wired control

Instructions of use

A	Rise backrest	E	Rise all sections simultaneously *(autocontour)*
B	Lower backrest	F	Lower all sections simultaneously *(autocontour)*
C	Rise legrest	G	Rise mattress platform
D	Lower legrest	H	Lower mattress platform

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD GESTIÓN DEL SERVICIO SANITARIOS · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.

ipardo

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)