AdvantCare Bed

Quick reference sheet

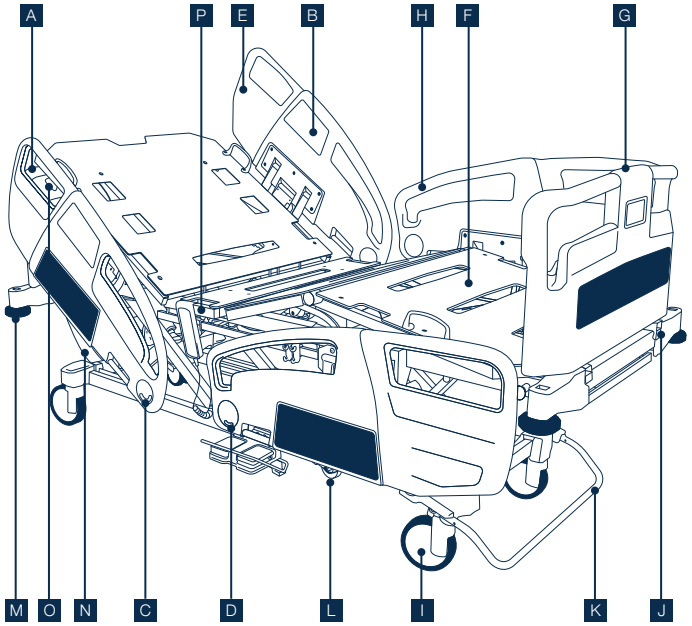

Bed's components

A	Removable curved headboard	I	Integral wheels Ø15 cm
B	Side rails membrane control	J	Headboard / footboard unlocking
C	Backrest tilting indicator	K	Centralised braking pedal
D	Trendelenburg / Reverse Trendelenburg tilting indicator	L	Directional fifth wheel (optional)
E	Backrest side rails	M	Bumpers
F	HPL mattress platform	N	Anchored headboard (optional)
G	Removable curved footboard	O	Emergency CPR handle
H	Legrest side rail	P	Fixed central HPL plane

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

sept 2024 | CódPCO753063_QuickSheet_AdvantCare_EN_2023_rev.01

Other functions

Side rails:

- Raising the rail: Pull the rail upwards until it is locked in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.

Emergency CPR:

- Activate either of the two levers located under the headrest module, accompanying it in turn as it lowers.

Centralised braking system:

- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in the middle position.
- Activating steering or 5th wheel: Pedal in raised position.

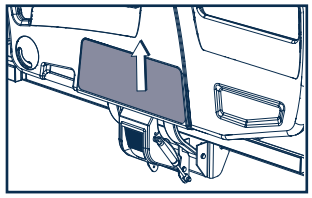

Raising the rails

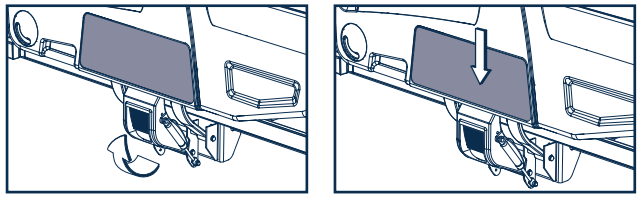

Lowering the rails

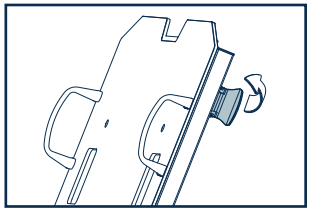

Emergency CPR



Brake



Free movement



Steering or 5th wheel

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails, headboard, footboard.

Cleaning and disinfection after a patient leaving or before a transfer:

- Mattress platform area, chassis of the bed.

Deep cleaning and disinfection every two months:

- Support and lifting area of the bed.

Maintenance

Always check the correct state of:

- Electrical wiring.
- Wheels.
- Braking mechanisms.

For more information, please consult the use and maintenance manual.

Controls

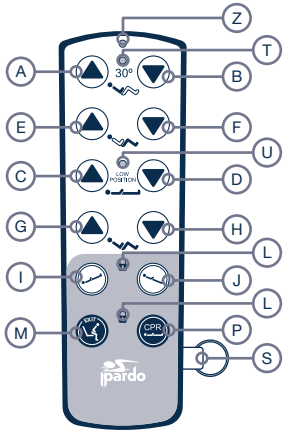

Patient control with locks

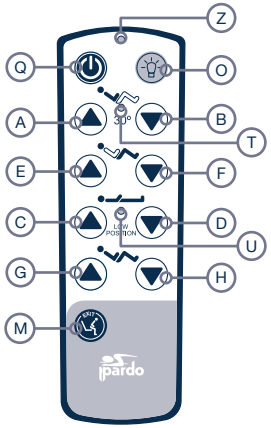

Patient control with light

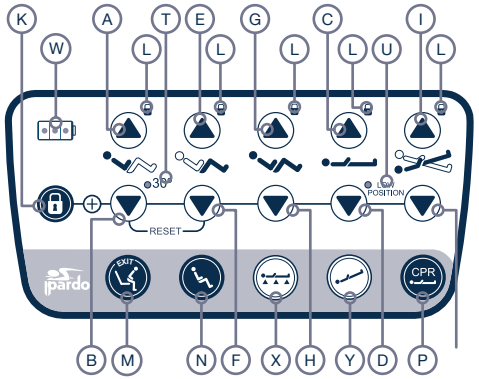

Wired nursing control

Instructions of use

A	Rise backrest	M	Safety Exit position
B	Lower backrest	N	Cardiac Chair position
C	Rise mattress platform	O	Light under bed
D	Lower mattress platform	P	Emergency CPR
E	Rise legrest	Q	Standby button
F	Lower legrest	S	Movement locking key
G	Rise backrest & legrest simultaneously *(autocontour)*	T	30º backrest indicator led
H	Lower backrest & legrest simultaneously *(autocontour)*	U	Low Position indicator led
I	Trendelenburg	W	Battery indicator
J	Reverse Trendelenburg	X	Exploration Position (maximum height)
K	Movements locking	Y	Emergency Trend position
L	Indicator led of locked movements	Z	Movement indicator led

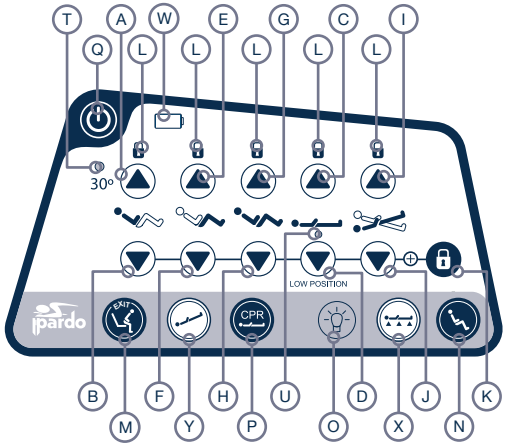

Advanced external membranes
(optional)

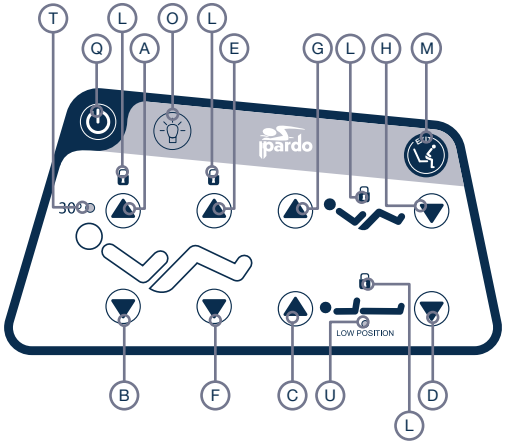

Simple external / inner membranes
(optional)

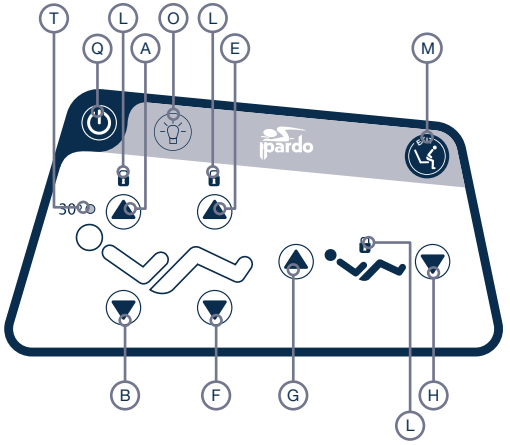

Simple external / inner membranes w/o lifting
(optional)

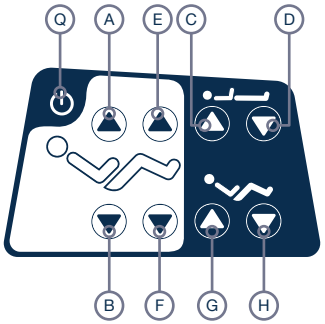

Basic external / inner membranes
(optional)

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR · AENOR · AENOR · AENOR · CE MD

SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)