Atica3404 Stretcher

Quick reference sheet

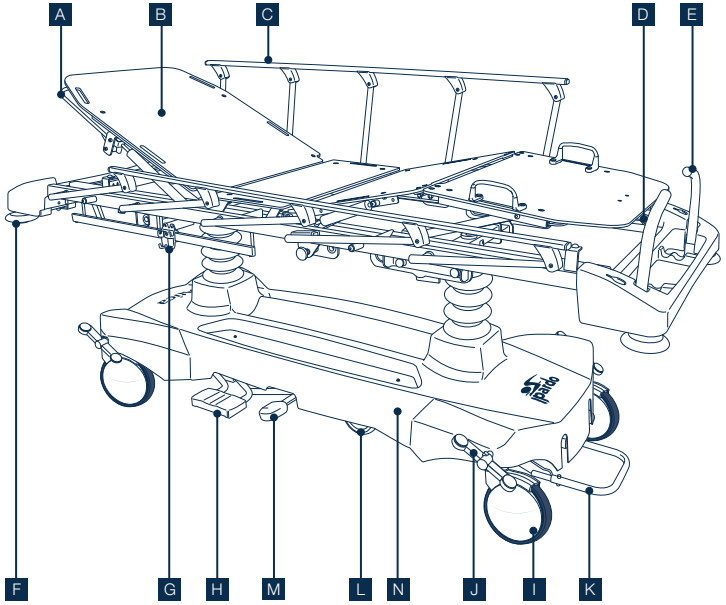

Stretcher's components

A	Backrest operating lever	H	Triple articulation pedal
B	HPL mattress platform*	I	Wheels Ø20 cm
C	Folding rails	J	Centralised braking pedals
D	Extremities operating lever	K	Fifth wheel actuation pedal
E	Carrying handles	L	Fifth wheel
F	Protective discs	M	Lifting pedal
G	Drainage holder hooks	N	Lower fairing

*Two or four articulated planes according to model.

www.pardo.es
TECHNICAL SERVICE CENTRE
(+34) 976 300 033

Other functions

Folding rails (1):

- Rail raising: Pull the rail upwards until it is locked in its highest position.
- Rail lowering: Pull the handle under the rails outwards. The rail lowers automatically.

Braking pedal (2):

- Braking the stretcher: Pedal in low position.
- Moving the stretcher: Pedal in the horizontal position.
- Steering wheel: Pedal in raised position.

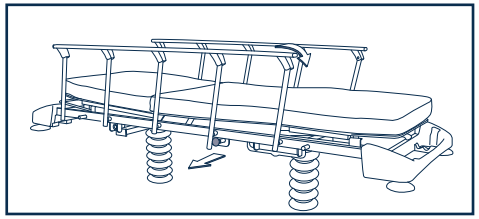

Raising rails

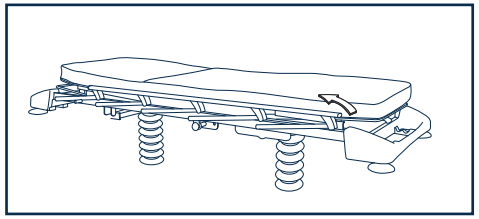

Lowering rails



Brake



Free movement



Steering wheel

Cleaning

Daily cleaning and disinfection with up to a 1000ppm concentration of chlorine solutions:

- Rails and carrying handles.

Cleaning and disinfection after a patient leaves or before a transfer:

- Stretcher platform, fairings, protective discs, levers and drainage holder hooks.

Thorough cleaning and disinfection every two months:

- The whole stretcher.

Maintenance

Always check the correct state of:

- Wheels.
- Braking mechanisms.
- Mechanical drives.

For more information, please consult the use and maintenance manual.

ene 2025 | Cód:PCO753134_QuickSheet_Atica3404_EN_2022_rev02

Mechanical operation

Raising and lowering the stretcher (1):

- Lifting: Stepping on the black pedal until the stretcher is at the desired height.
- Lowering: Depressing continuously the centre of the grey pedal.

Trendelenburg / Reverse Trendelenburg (2):

- Trend: Stepping on the grey pedal from the backrest closer side makes the column descend in a controlled way and reaches the desired height.
- Antitrend: Stepping on the grey pedal from the footrest closer side. Press the lift pedal to return the stretcher to its original position.

Fifth wheel (3):

- Operate by pressing the rear pedal located in the footboard area and deactivated by lifting it.

Backrest section (4):

- Press the hand lever manually along with the module to facilitate both raising and lowering.

Extremities section (5):

- Pull the lever underneath the extremities module and manually move it to the desired position.

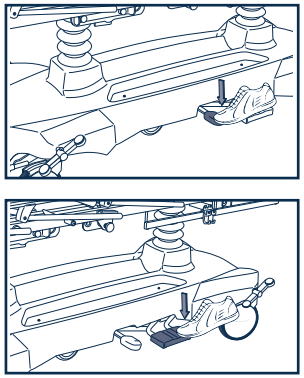

Raising and lowering pedals

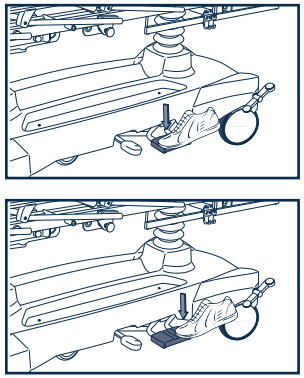

Trend / Rev. Trendelenburg

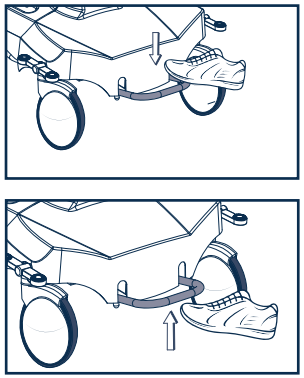

Fifth wheel



Backrest section

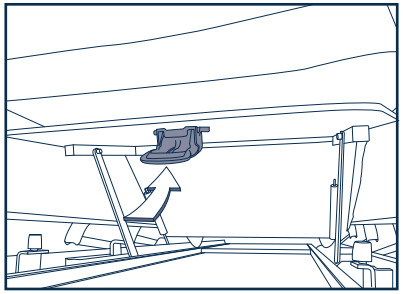

Foot section

Accessories

Foldable drip support incorporated:

- Telescopic rod for easy installation in the upper part of the stretcher. With height adjustment and 4 kg holding capacity.

Fixed drip support:

- Easily removable and can be attached to the 4 corner anchorage systems.

Drainage holder hooks:

- Located in the rings on the sides of the stretcher, on the underside of the chassis.

X-ray cassette tray:

- Reduces patient transfer tasks and the workload of healthcare personnel.

Monitor holders:

- Table anchored to the accessory supports of the stretcher handles.

Paper roll holder

- It is placed in the footboard area of the stretcher and attached to the stretcher in the accessory supports.



Foldable drip support incorporated



Fixed drip support



Drainage holder hooks



Paper roll holder



X-ray cassette tray



Monitor holders

Industrias Hidráulicas Pardo S.L. company has the following certifications:

IQNET LTD · AENOR GESTIÓN DE LA CALIDAD · AENOR GESTIÓN CALIDAD GESTIÓN DE SERVICIOS SANITARIOS · AENOR GESTIÓN AMBIENTAL · AENOR ECODISEÑO · CE MD

SAFETY WARNINGS

- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.

Industrias Hidráulicas Pardo, S.L. C/ Los Ángeles 5, (Polígono Centrovía) - 50198 La Muela, Zaragoza (Spain)